

Artmex

MTS & PMU System


V11



User Manual



No.	Description
1	Hand-piece placement area
2	Pedal interface
3	Hand-piece interface
4	Power interface
5	Power switch
6	Pedal

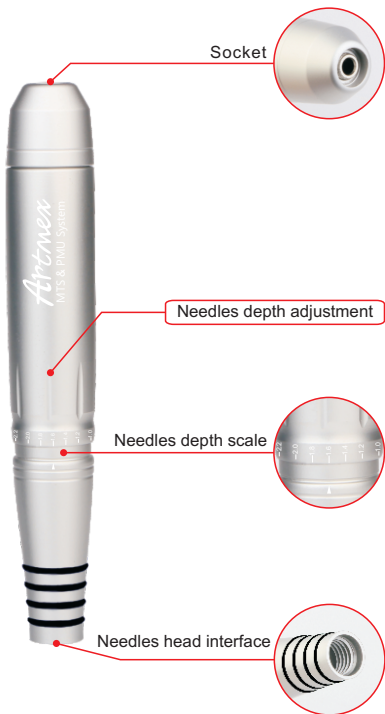

PMU marks the color pigments inhale into the needle by injecting them to skin by a back-and-forth motion
MTS helps medical supplies be absorbed to skin by irritating

Basic Operation

1. Connect accessories to the Artmex V11 main body



Fig 1



Power

Fig 2

Cord of adapter connects to power interface
(See fig 1 and fig 2)



Fig 3



Pen

Fig 4

Cord of hand piece connects to hand piece interface
(See fig 3 and fig 4)



Fig 5



Pedal

Fig 6

Cord of pedal connects to pedal interface
(See fig 5 and fig 6)

2. Plug DC adapter to AC outlet
3. Turn on the power switch to enter interface as(Fig 7)



Fig 7

4. Click the interface(Fig 7) to enter interface as(Fig 8)

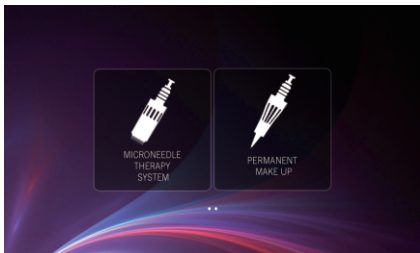


Fig 8


5.Mode selection. Click “” to enter the interface as(Fig 9)



Fig 9



No.	Description
1	Level
2	Speed Adjustment (up)
3	Start/Pause Button
4	Speed Adjustment (down)
5	Return key
6	Speed
7	Shutdown button
8	Time frame setting

6. Install the needles cartridge. Selectable disposable needle cartridge between MTS and PMU for its purpose


7. Click **+** or **-** to select the speed level
10 speed levels. Higher level, higher speed
The pen will stop working when the speed level is "0"

8. Click **▶||** to make the pen start working **Or use pedal to control the hand-piece.**

9. Adjust the needles depth(Maximal depth is 3.0mm)
Needles depth adjustment should be done after the pen working

Operation Of PMU mode.

The operation of PMU is the same with MTS after choose the mode.

Click "" to enter the interface as(Fig 10)

PERMANENT
MAKE UP

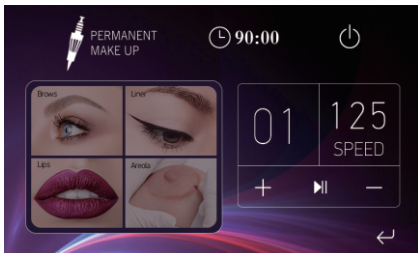



Fig 10

Choose suitable operation mode according to purposes of usage

Click the  and the interface will show like Fig 11

- EYE BROW: The speed starts from level 6

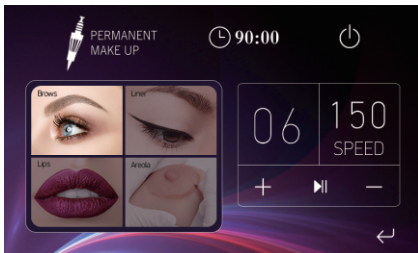



Fig 11

Click the  and the interface will show like Fig 12

- EYE LINE: The speed starts from level 4

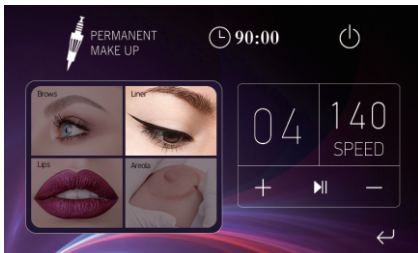


Fig 12

Click the  and the interface will show like Fig 13

- LIPS: The speed starts from level 6

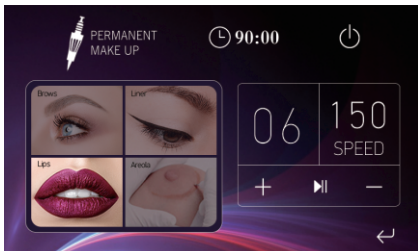



Fig 13

Click the  and the interface will show like Fig 14

- AREOLA: The speed starts from level 5

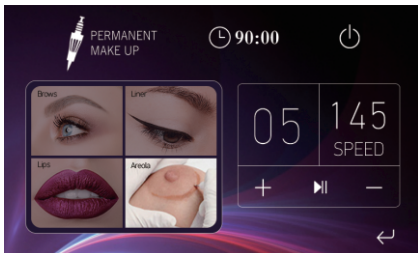



Fig 14

Click  to enter the interface as (Fig 15)

The default time is 90 minutes.

The maximal time is 99 minutes.

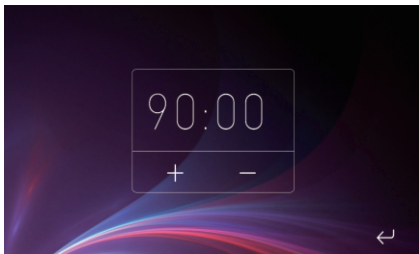


Fig 15

Turn off the machine


Click  to enter the interface as (Fig 16)



Fig 16

Using the stylus to touch the screen 10




Fully automated intelligent hand piece



During the working state. When the pen stays on the place area of pen, it stops working automatically.


During the working state. When the pen leaves the place area of pen, it starts working automatically.

- (1) Take out needles cartridges in the sterilized packing
- (2) Pushing the needle cartridge horizontally into the round slot of pen
- (3) Assemble the needles cartridges by clockwise rotation
Take apart the needles cartridges by counterclockwise rotation
- (4) Adjustment of needle length should be done after turn on the machine



Adjustment of needles depth

Adjusting the depth of needle by turning the needles depth adjustment. Turn it clockwise, needle depth will be longer. Turn it counterclockwise, needles depth will be shorter

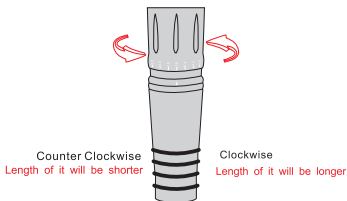



M1



L1



R3-M



R3-L



R5



F3



F4



F5



F7



F9



S3



S5



V9



V12



M9



M12



M24



M36



M42



Nano



P18

Product information	
Classification	Contents
Model name	ARTMEX-V11
Patented product	Yes
Purpose of Use	Permanent make-up & Micro-needle Therapy
Aadpter	100V~240V
Weight	2900g
Size	420mm*295mm*105mm

Package List

Item	Quantity
Host	1 pc
Hand piece	1 pc
Adapter	1 unit
Pedal	1 unit
Stylus	1 pc






















Maintenance

1. General maintenance

- Keep it with its power off. Wipe its surface out with a dry cloth
- Keep it away from direct sunlight or high temperature and humidity.
- Do not leave the measurement, repair or alter of the device to ' non-professional staff.

2. Routine inspection

- Make sure to inspect the device and adapter before use.
- When you use the device which has not been used for a long time, make sure to check if it works properly with safety

	Alternating current		Serial No
	Direct current		EU Representative
	Class II equipment		CE mark
	Attention, consult accompanying documents		Manufacturer
	Date of manufacture		Floating applied part
	Please be sure to read instructions before use and follow as described.		
	<p>Do not apply it to the man as follow:</p> <ol style="list-style-type: none"> 1. Who has acute disease or bloody disease over 38°C 2. Who has allergy and hemophilia 3. Who has melanosis of the face 4. Who has high internal heat 5. Who regularly visits hospital 6. Who takes medicines 7. Who is under 12 years old 		
	Do not use it on the power other than AC 220V. It may cause fires or malfunction		
	Do not use it near the place with high temperature, dust or humidity (Near the humidifier). It may cause malfunction.		
	Do not repair, disassemble or alter the controller and the body. It may cause malfunction.		
	Do not touch the device or detach the power cords with wet hands. It may cause electric shock.		
	Do not use the stripped cord or propped cord. It may cause fires(Be sure to replace it with another).		
	Do not use the propped cord which has crack or scares. It may cause scares on the skin.		
	When you don't use it for a long time, unplug it from the outlet.		
	Be sure to have an inspection for test. If any troubles are found, get it repaired.		
	No one other than the operator can touch it. It may cause accidents or malfunction.		



Artmex
MTS & PMU System