



MITS FRANCE	Ċ	
Million 150 Seco	MTS Areola	J.
+ 1 * 1 -	Lipliner Eyeliner	
Ęy	ebrows	
	P	

# **User Manual**



Product detail	1
Basic operation	3
Intelligent hand-piece	5
Needles head installation	6
Adjustment of needles depth	6
Needles head introduction	7
Specification	8
Precaution	9





- Speed up
- ③ Speed down
- 5 Power switch
- ⑦ Power interface

- (2) Start/Pause button
- ④ Function keys
- 6 Pedal
- 8 Hand piece interface






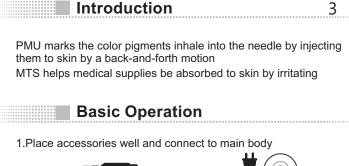

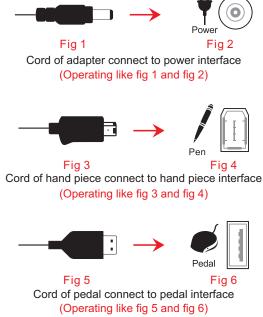

2.Plug DC charger to AC outlet

3.Click () to turn on the machine and it shows like Fig 7



### Fig 7

- 4. Choose the mode on the menu. The icon will flash after clicking the function key.
- 5.Click to select the speed level

### 11 speed levels. Higher level, higher speed

6.Click to start or pause the hand-piece.

Or use pedal to control the hand-piece.

## Automated intelligent hand piece 5

### **Stationary mode**



The pen will stop working automatically when it stays on the placement area.

### **Operating mode**



The pen will start working automatically when it leaves the placement area.

- 1. Take out needles cartridges from the sterilized package.
- 2. Pushing the needle cartridge horizontally into the round slot of pen.
- 3.Assemble the needles cartridges by clockwise rotation take apart the needles cartridges by counterclockwise rotation.
- 4.Adjustment of needle length should be done after turning on the machine.




# Adjustment of needles depth

Adjusting the depth of needle by turning the needles depth adjustment.

-Turn it clockwise, needle depth will be longer. -Turn it counterclockwise, needle depth will be shorter



# **Needles head introduction**

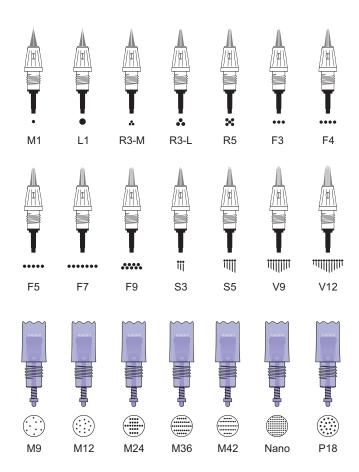

# [Model name] : ARTMEX - V9 [Weight] : 2100g [Adapter] : 100V~240V [Size] : 290mm\*273mm\*105mm [Patented product] : Yes [Purpose of Use] : Permanent make-up & Micro-needle Therapy

# Maintenance

Specification

### 1.General maintenance

-Keep it with power off. Wipe its surface up with a dry cloth.-Keep it away from direct sunlight or high temperature and humidity.-Do not leave the measurement, repair or alter of the device to non-professional staff.

### 2.Routine inspection

-Make sure to inspect the device and adapter before use.

-When you use the device which has not been used for a long time,

make sure to check if it works properly with safety.

# Package list

Host	1 pc	
Hand piece	1 pc	
Adapter	1 pc	
Pedal	1 pc	

$\sim$	Alternating current	SN	Serial No		
	Direct current	EC REP	EU Representative		
	Class II equipment	Œ	CE mark		
$\triangle$	Attention, consult accompanying documents	-	Manufacturer		
M	Date of manufacture	F	Floating applied part		
$\bigcirc$	Please be sure to read instructions before use and follow as described.				
	Do not apply it to the man as follow: 1.Who has acute disease or bloody disease over 38 °C 2.Who has allergy and hemophilia 3.Who has high internal heat 4.Who has high internal heat 5.Who regularly visits hospital 6.Who takes medicines 7.Who is under 12 years old				
$\bigcirc$	Do not use it on the power other than AC 220V. It may cause fires or malfunction				
$\bigcirc$	Do not use it near the place with high temperature, dust or humidity (Near the humidifier).It may cause malfunction.				
$\bigcirc$	Do not repair, disassemble or alter the controller and the body. It may cause malfunction.				
$\bigcirc$	Do not touch the device or detach the power cords with wet hands. It may cause electric shock.				
$\bigcirc$	Do not use the stripped cord or propped cord. It may cause fires(Be sure to replace it with another).				
$\bigcirc$	Do not use the propped cord which has crack or scares. It may cause scares on the skin.				
$\bigcirc$	When you don't use it for a long time, unplug it from the outlet.				
$\bigcirc$	Be sure to have an inspection for test. If any troubles are found, get it repaired.				
$\bigcirc$	No one other than the operator can touch it. It may cause accidents or malfunction.				